


Recycling Separation of Tea Methanol Extracted products

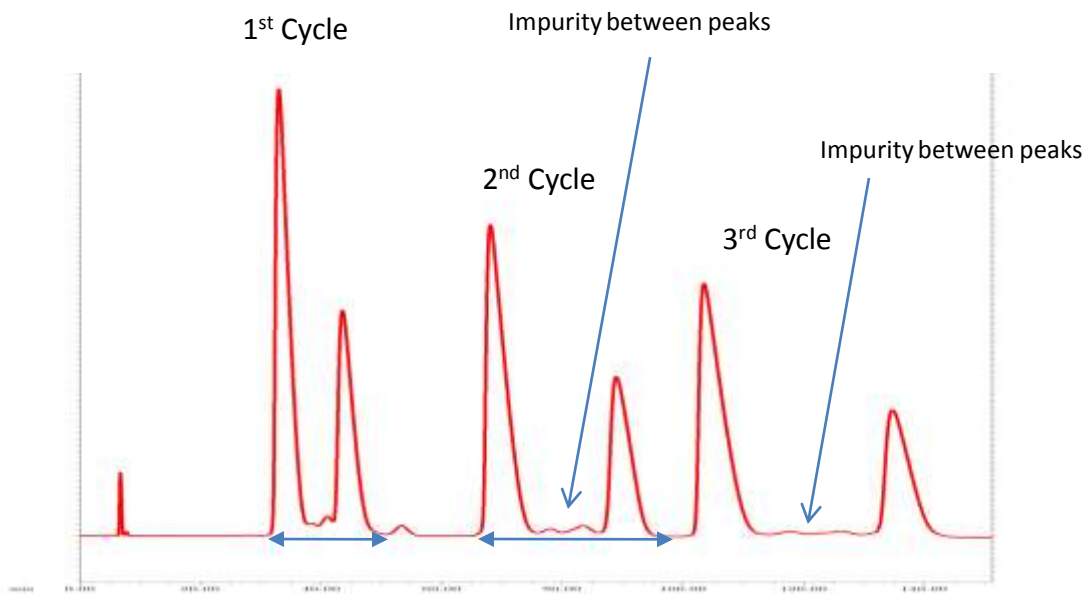

Column: JAIGEL-ODS-AP, SP-120-15
Eluent : 0.1 % Formic acid/ACN (83/17)
Flow rate : 9.0 ml/min
Detector : UV-310 @ 220 nm
Sample : 30 mg/3 ml