


Recycling Separation

Phthalocyanine position isomer



- Column: JAIGEL-GS310
- Detector: @254 nm
- Eluent: 100 mM NaClO
in Water/Methanol (10/90)

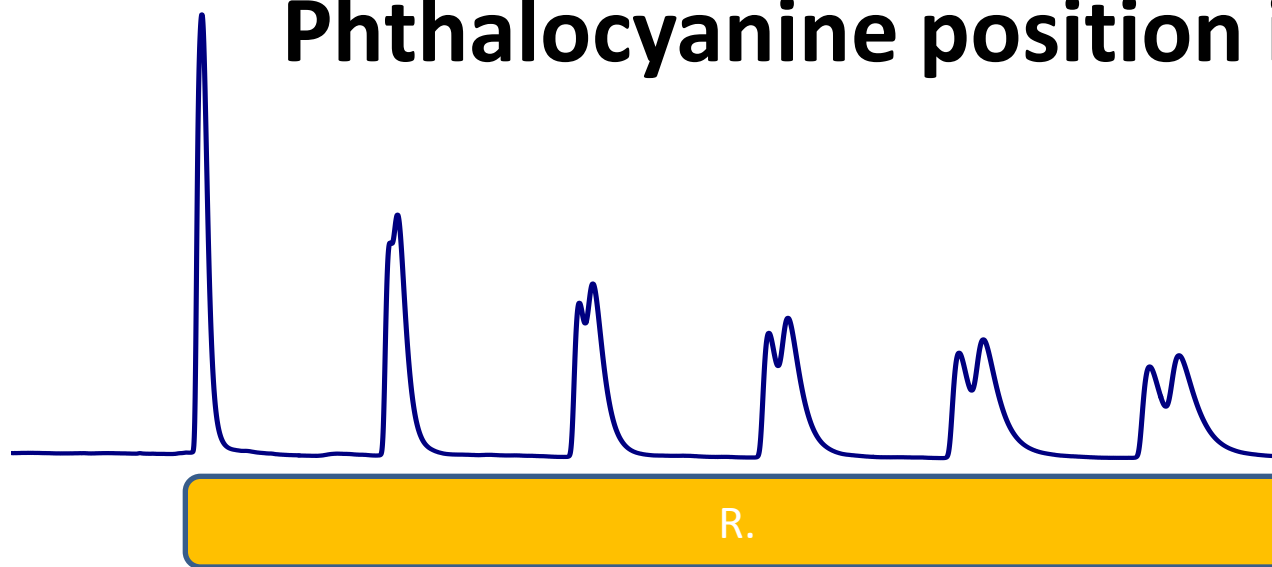