





Curie Point Injector JCI-22 VOC Analysis From Leaf

Purge gas out

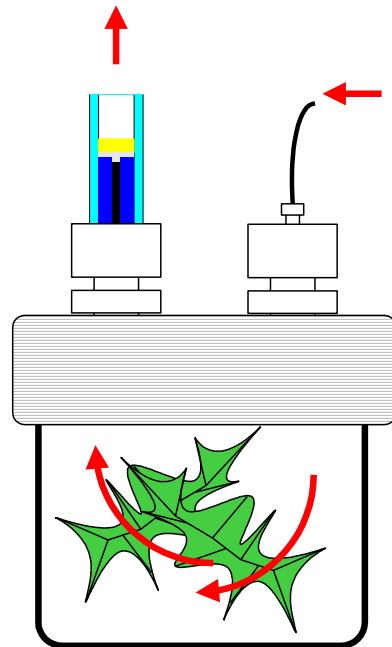


Purge gas in

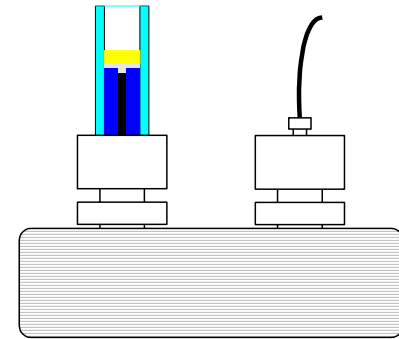



mini-PAT

Quartz Glass Sample Tube
ID: 4mm Length: 36mm
Absorbent :Tenax GR 25mg
Pyrofoil :F280

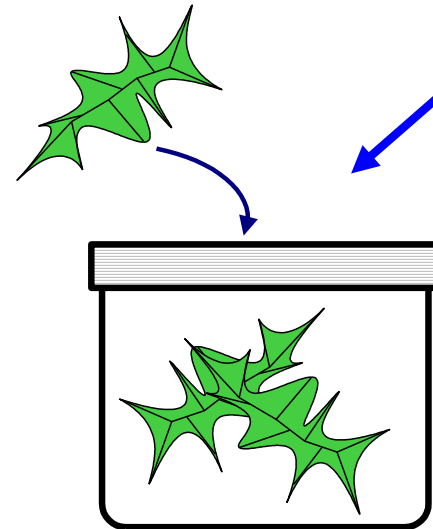

JCI-22
JAS-15M II

Japan Analytical Industry Co., Ltd

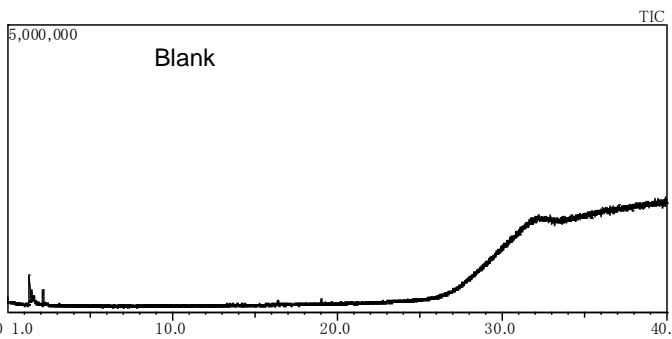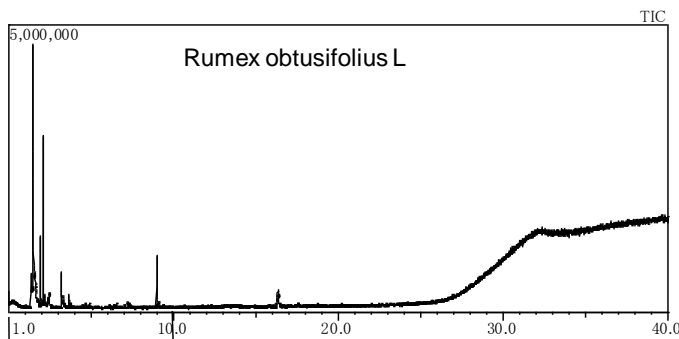

Broad-leaved dock

拡大
RT: 0-10 min

